

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906




Date: 07/19/2023

BFO

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:57
INTERNAL STANDARD	VERIFIED	18:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	18:57
BLANK TEST	0.00	18:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:00
BLANK TEST	0.00	19:00

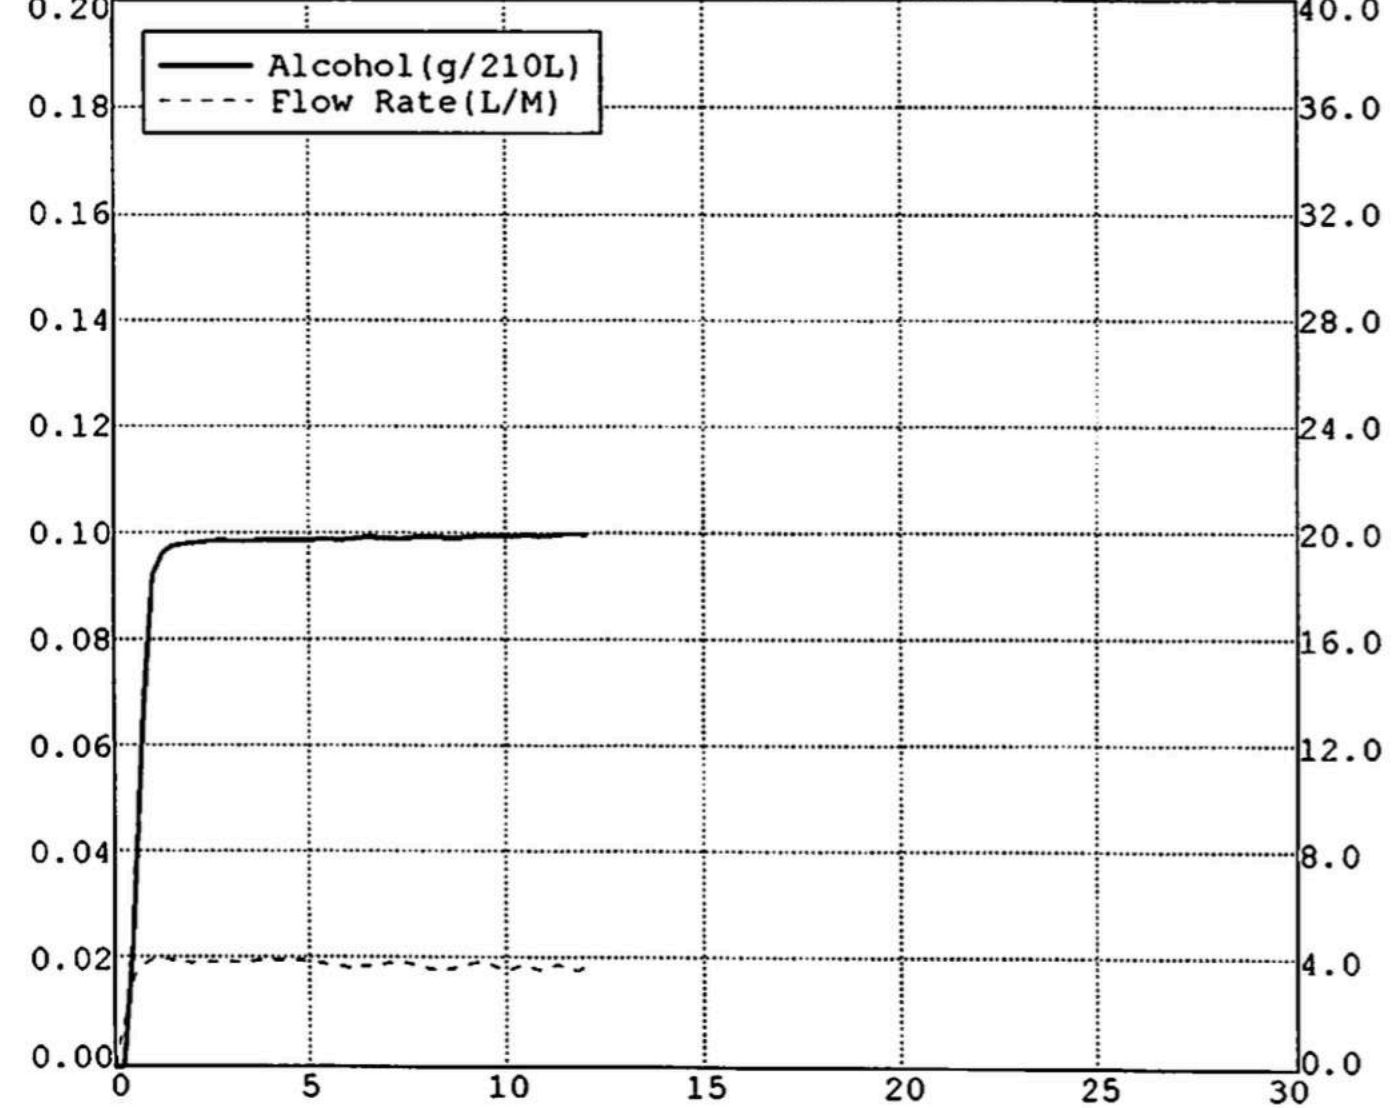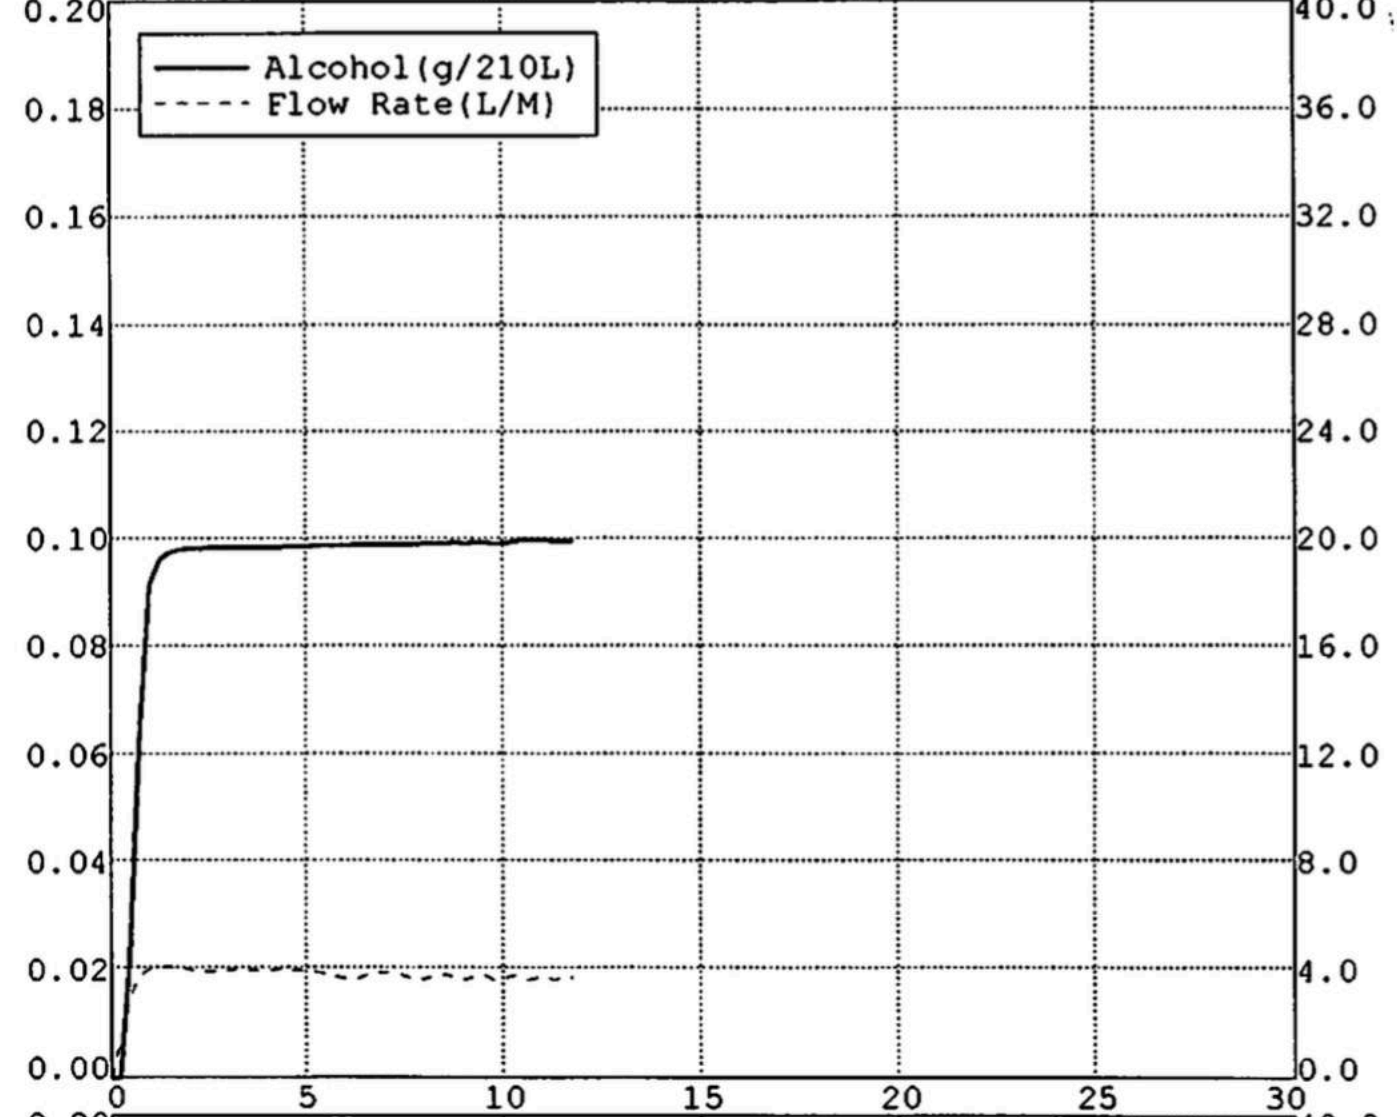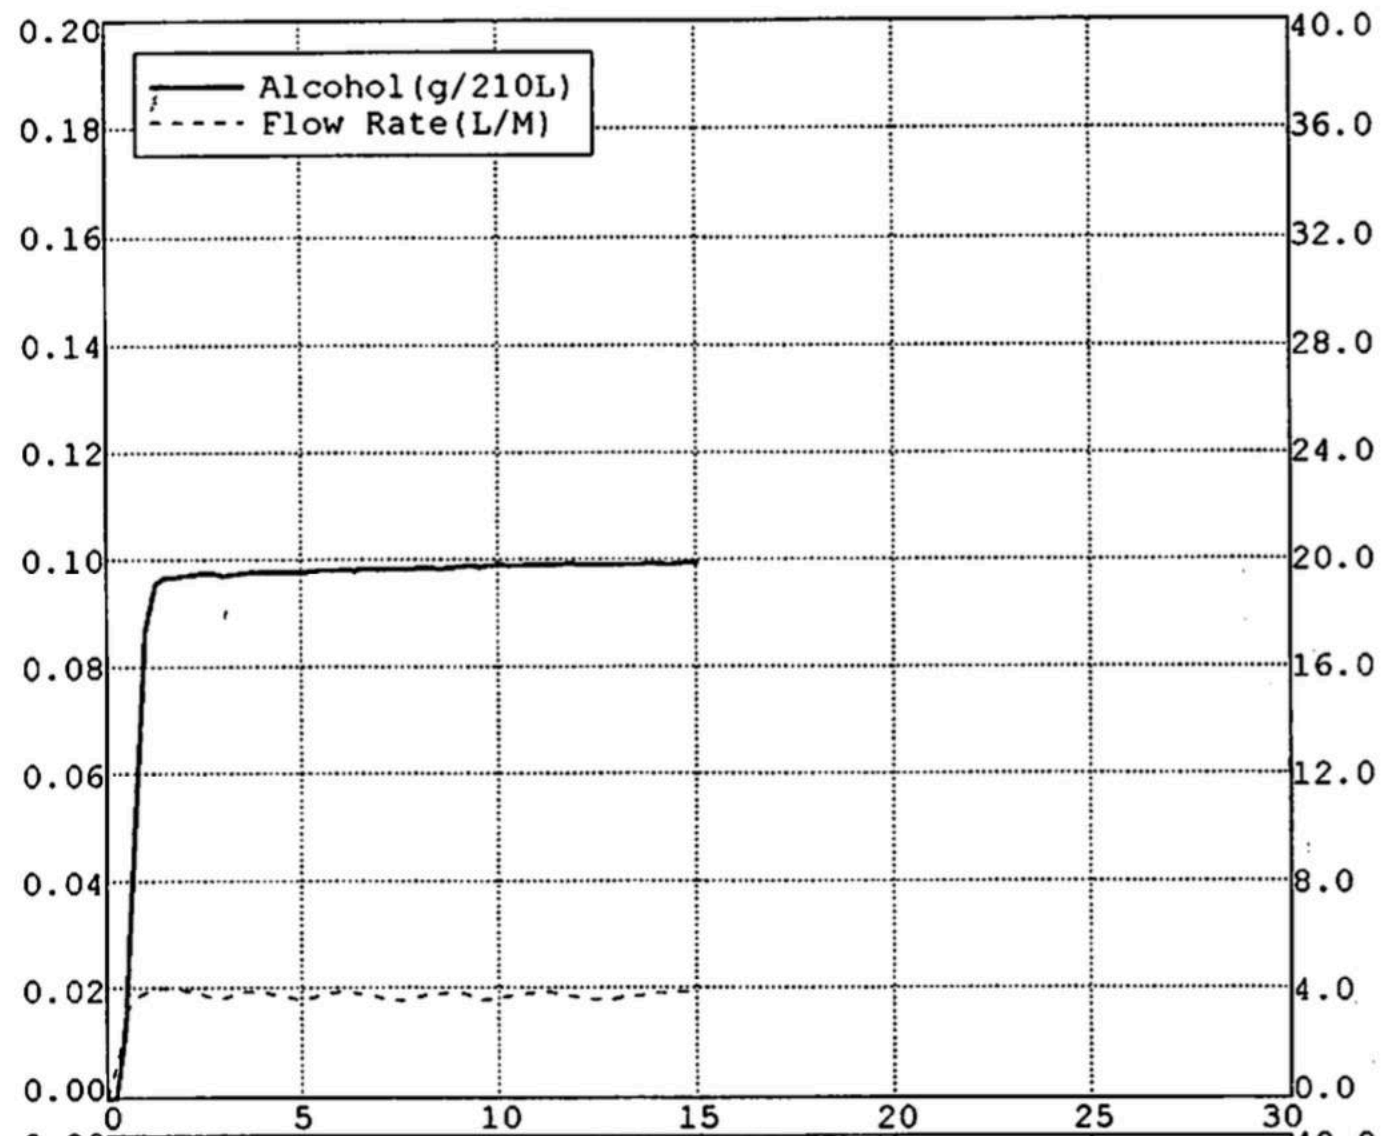

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 07/19/2023

OPERATOR NAME:
KRISTY N ALLEN
Permit #: 49726
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:40
INTERNAL STANDARD	VERIFIED	05:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	05:41
BLANK TEST	0.00	05:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	05:42
BLANK TEST	0.00	05:43
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	05:43
BLANK TEST	0.00	05:44

