

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 07/21/2021

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:43
INTERNAL STANDARD	VERIFIED	20:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:43
BLANK TEST	0.00	20:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:44
BLANK TEST	0.00	20:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:46
BLANK TEST	0.00	20:47

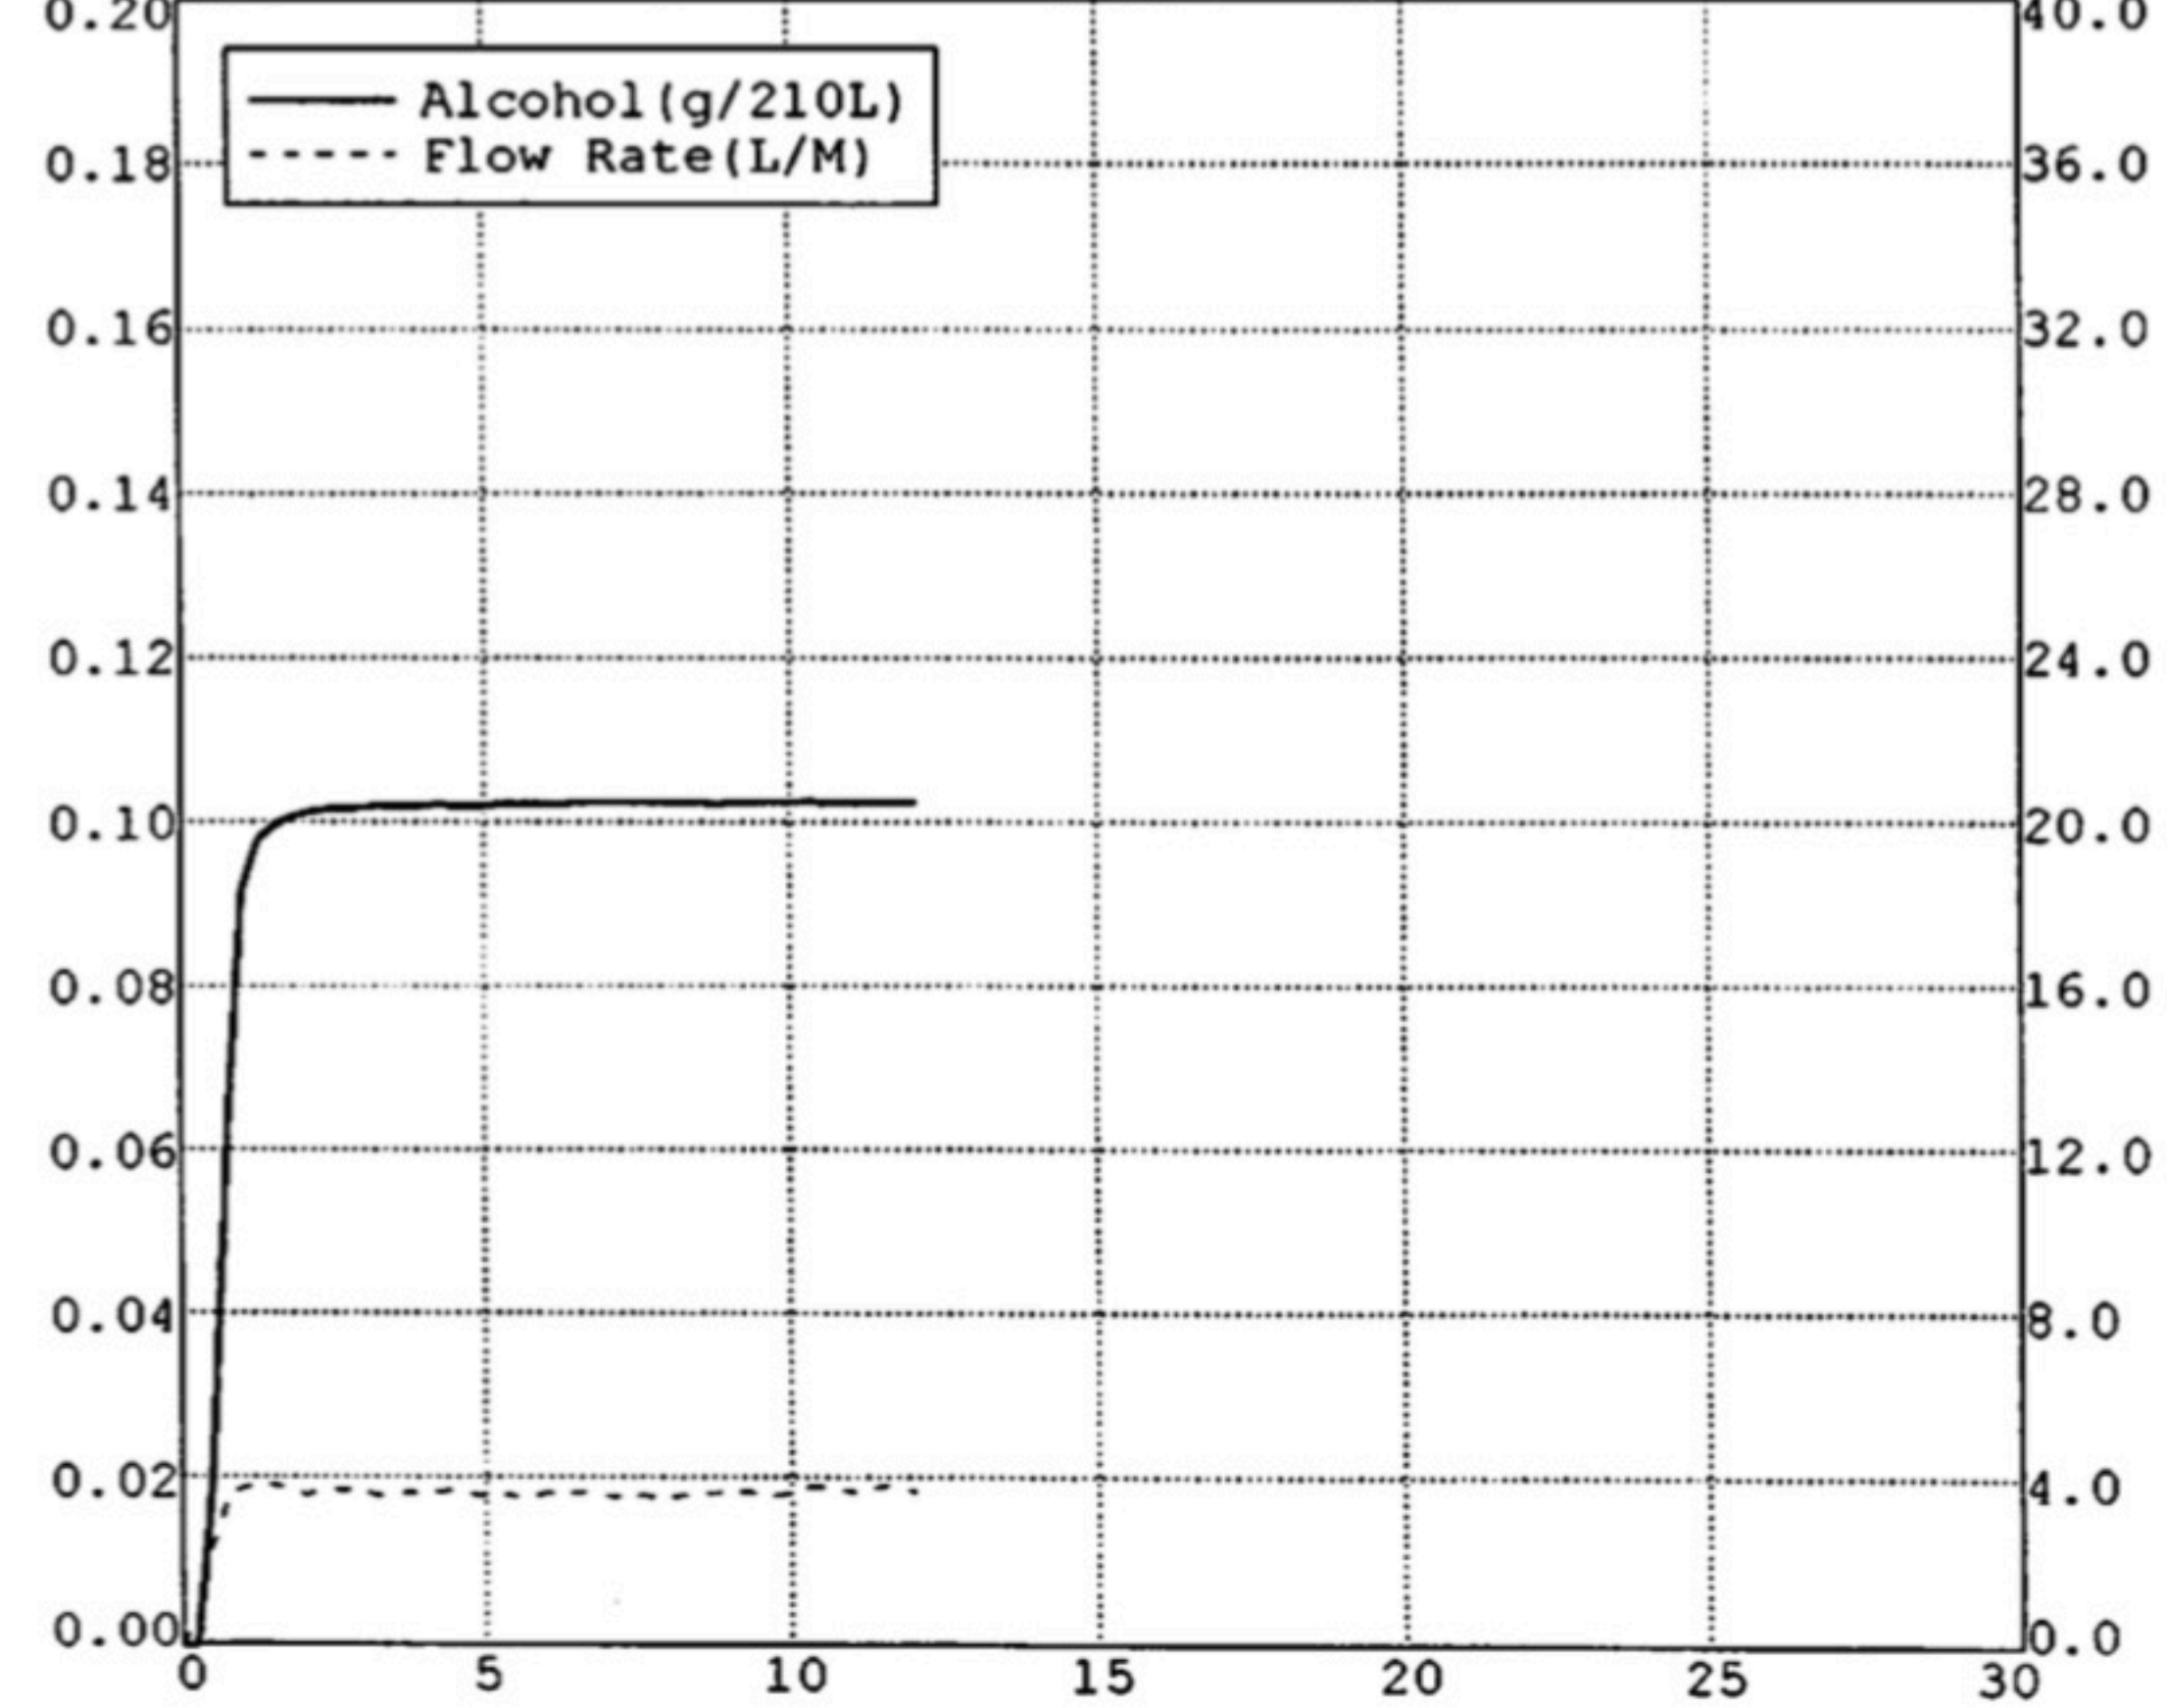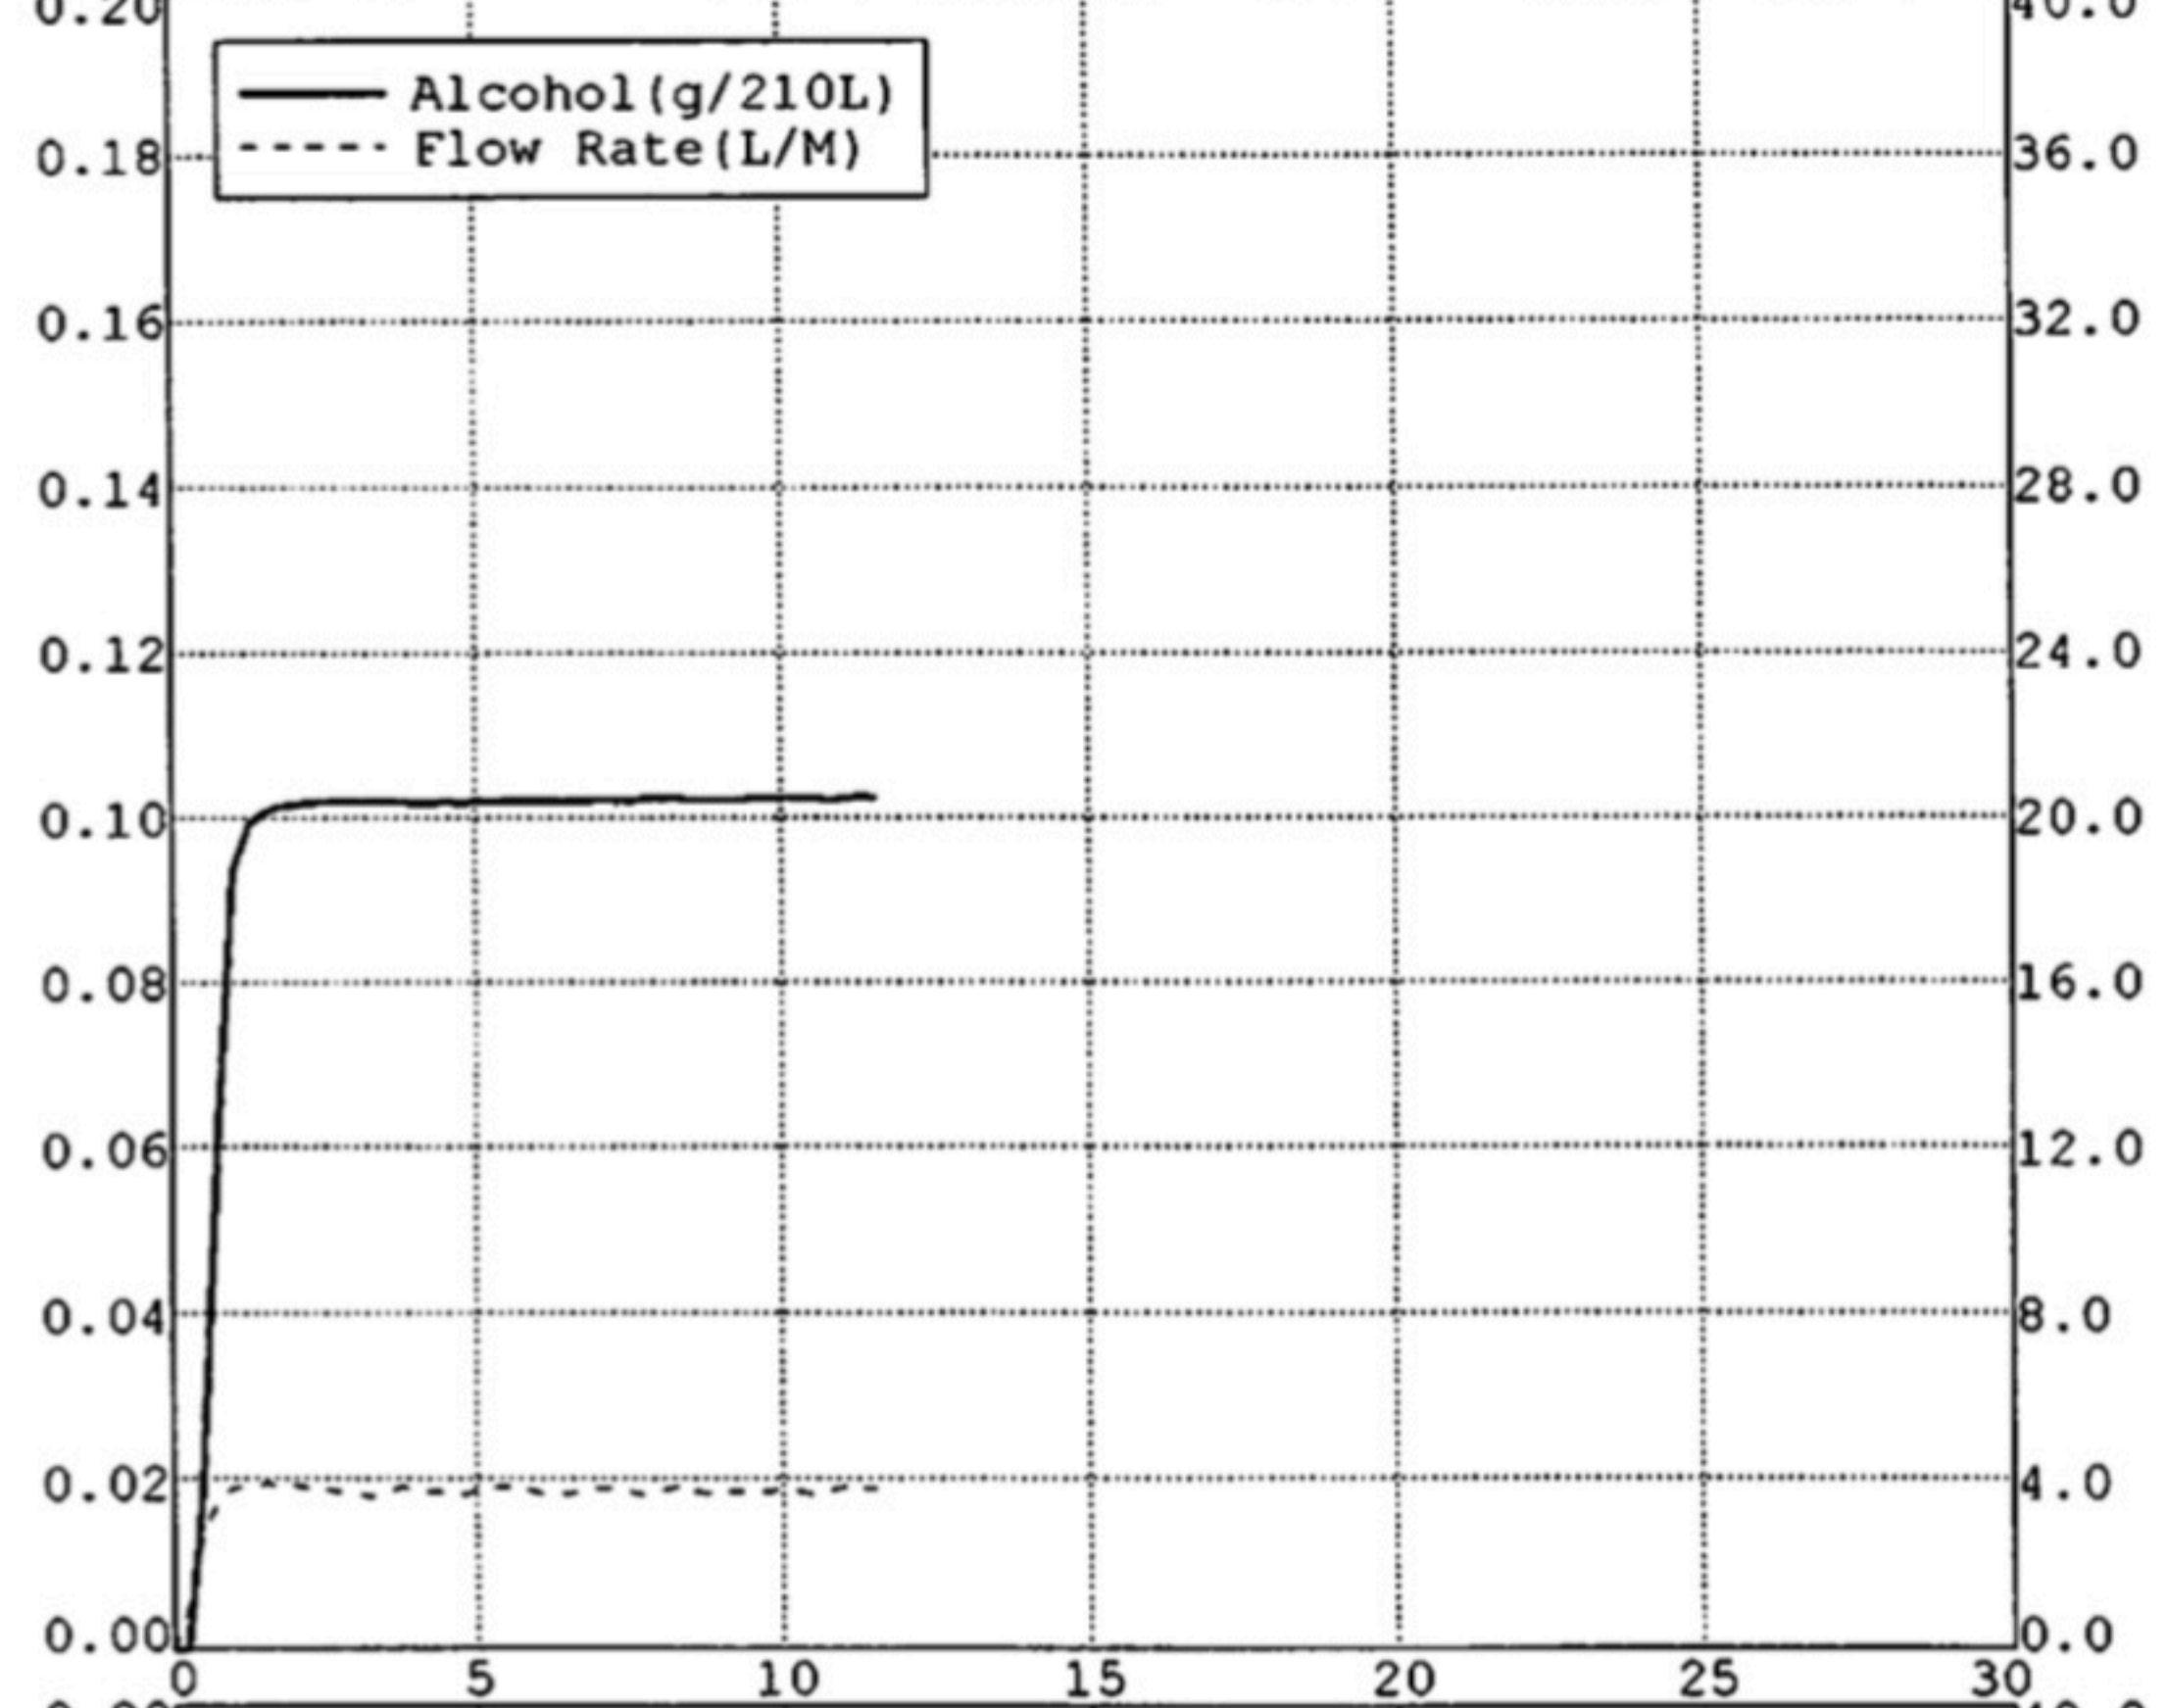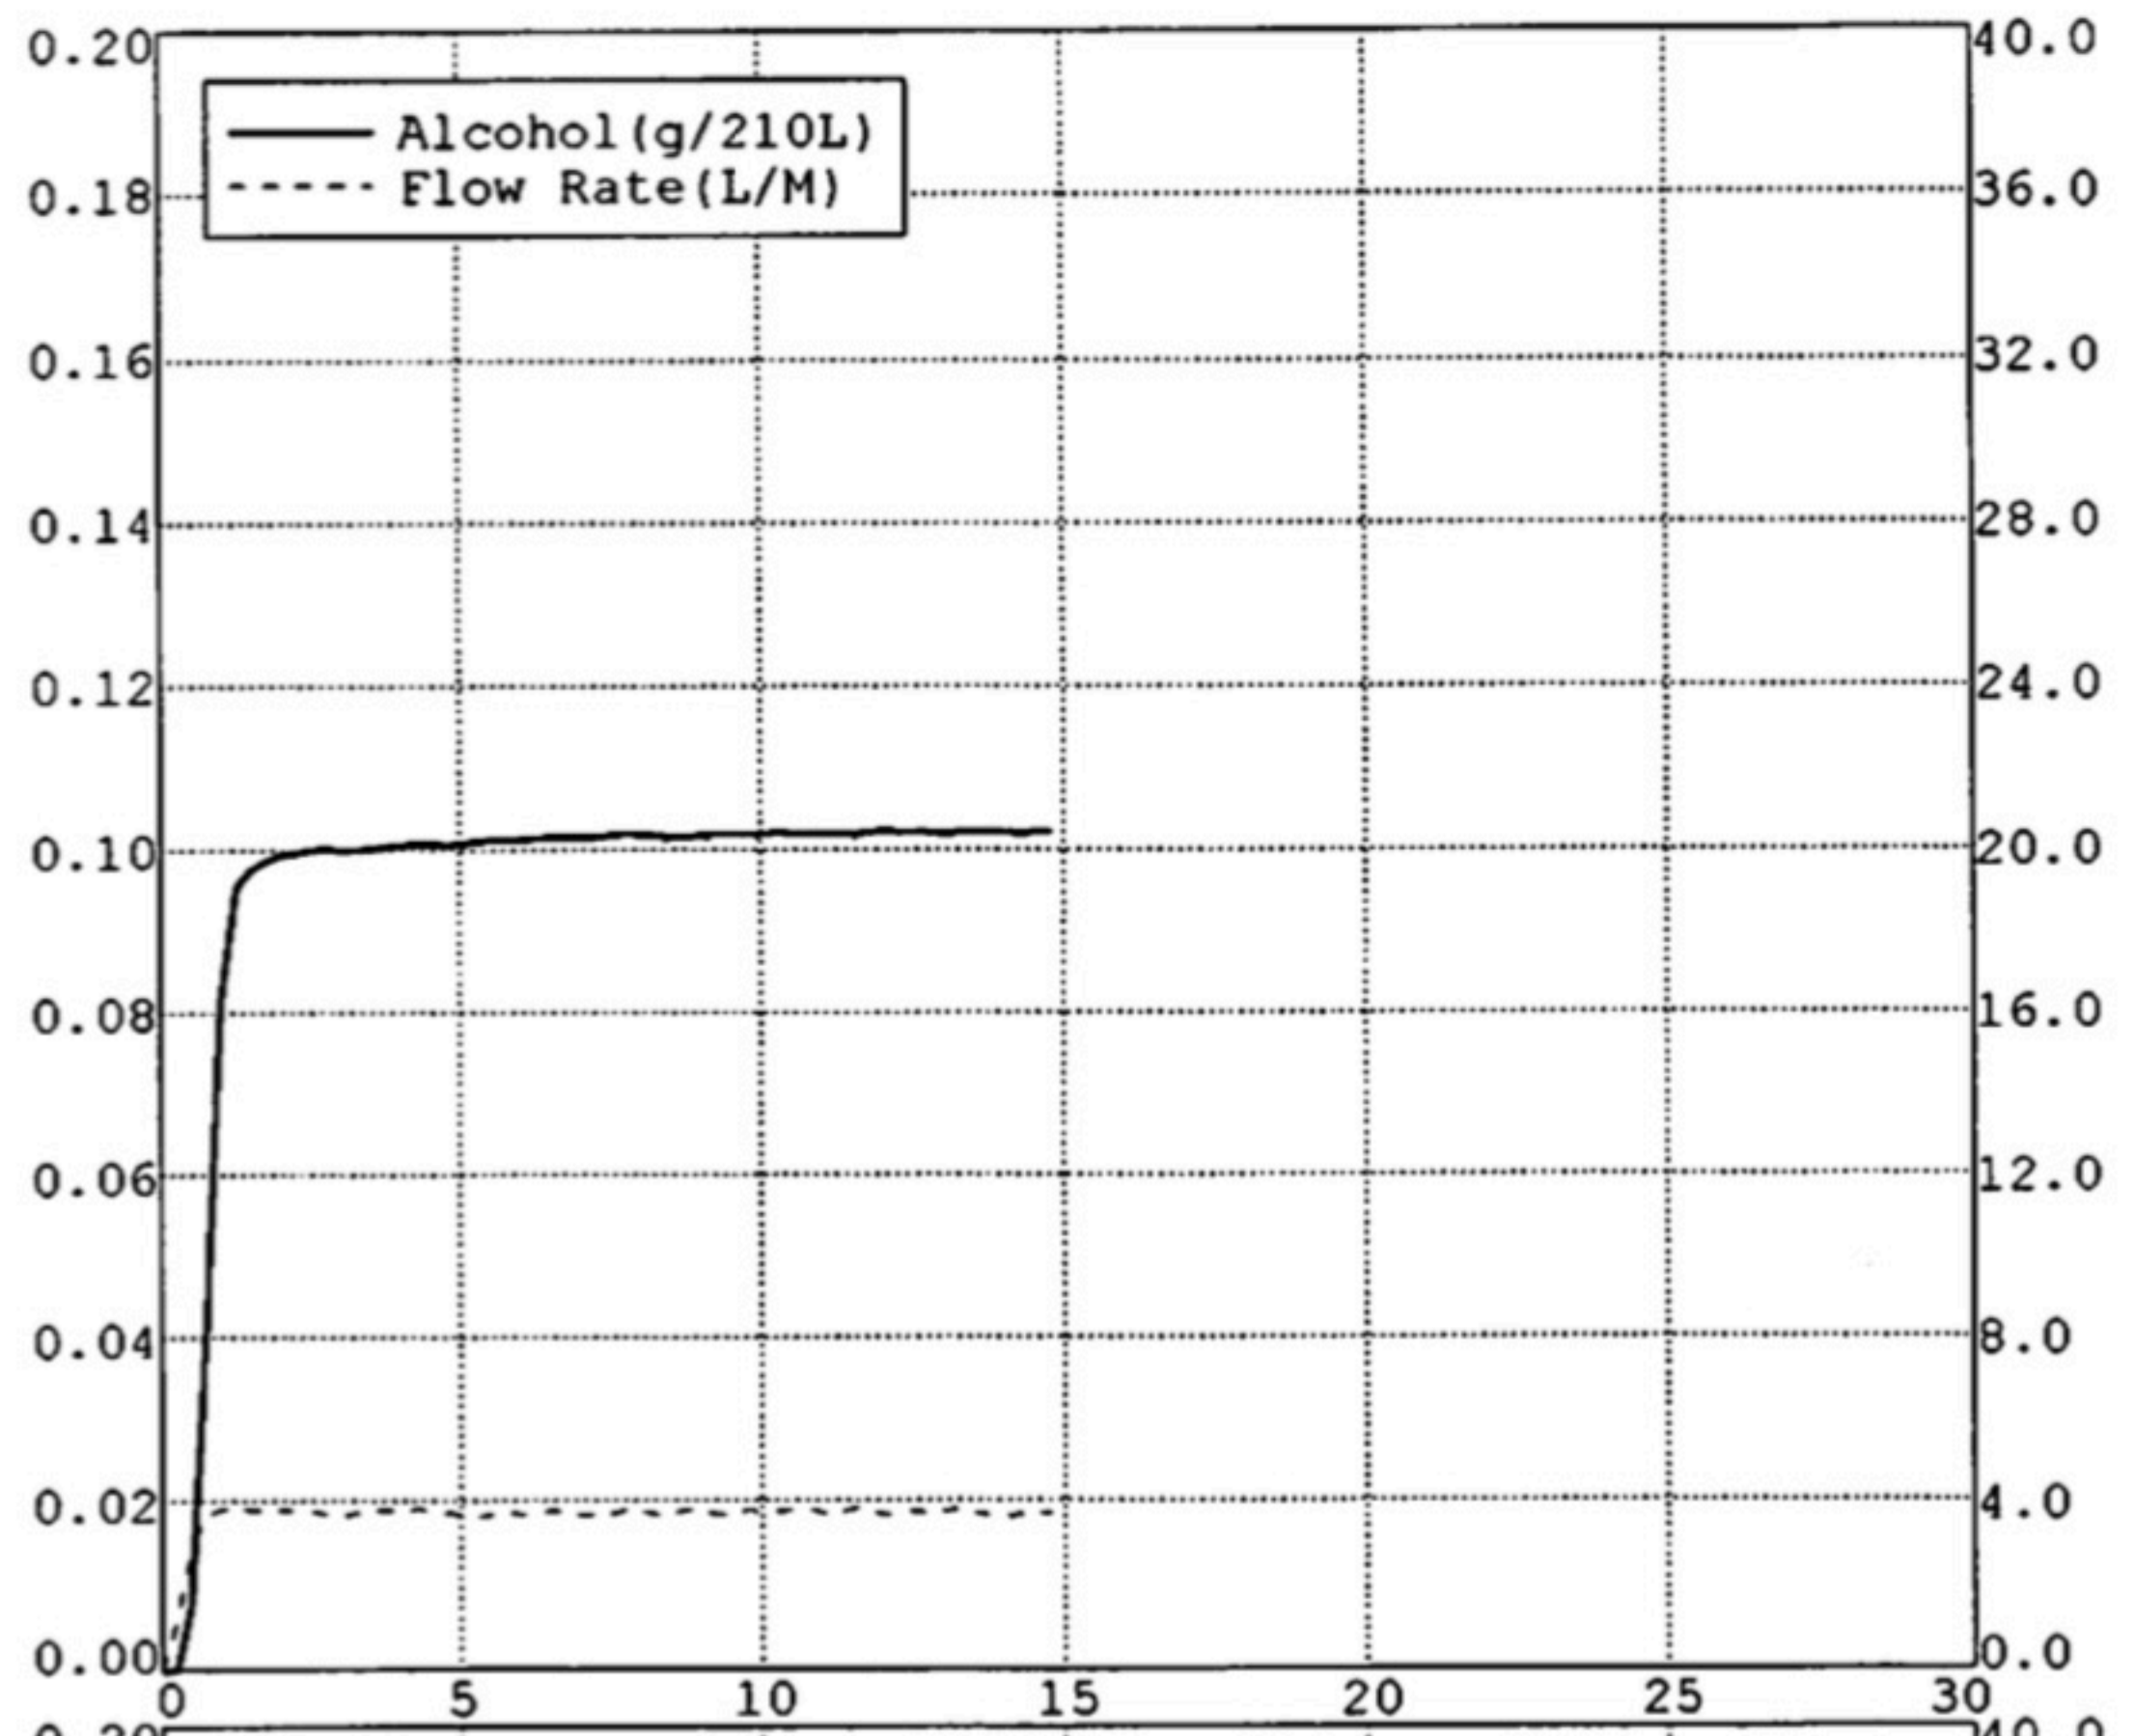

SUPERVISOR TEST

WFO

ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 100197

Date: 07/29/2021

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. S.O.
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:03
INTERNAL STANDARD	VERIFIED	04:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:03
BLANK TEST	0.00	04:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:05
BLANK TEST	0.00	04:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:06
BLANK TEST	0.00	04:07

